

SAMPLE RECEIVED
July 16, 2026

COA ISSUED
July 21, 2026

SAMPLE INFORMATION

Vendor
Aurevia Bioscience

Sample Name
B-Water 3mL

Sample Type
Clear liquid

Lot Number
00011

MW (g/mol)
91.1

ANALYTICAL METHODS

Identity: Confirmed via LC-MS/MS




Purity: RP-HPLC (214 nm)

Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: B-Water	Benzyl Alcohol	LC-MS/MS	✓ Conforms
Content	1.001 %	HPLC Quantitation	✓ Conforms
Overall Purity	99.8%	RP-HPLC (214 nm)	✓ Conforms
pH	8.35	<pH Meter>	✓ Conforms

HPLC Chromatogram · Retention Time 5.993 min

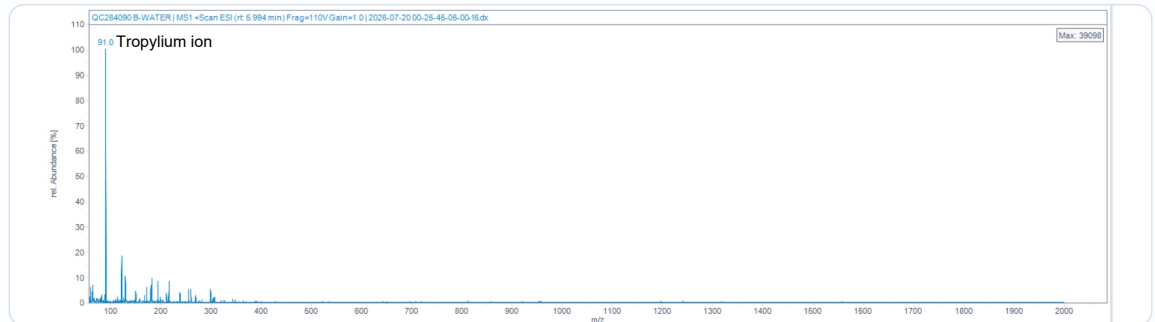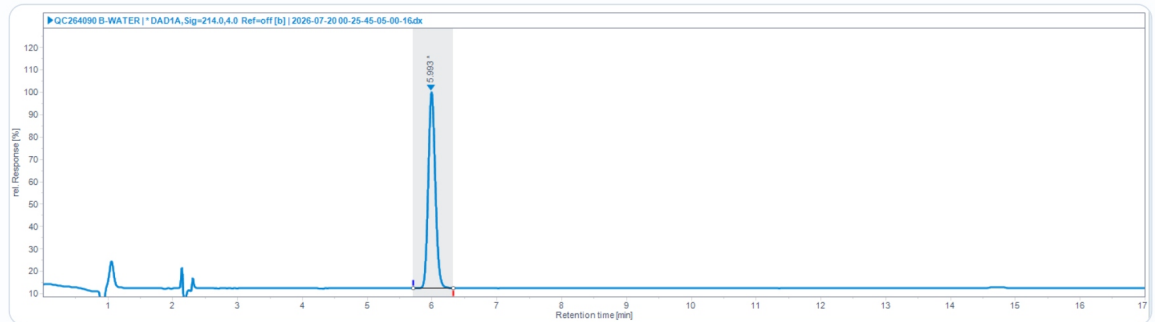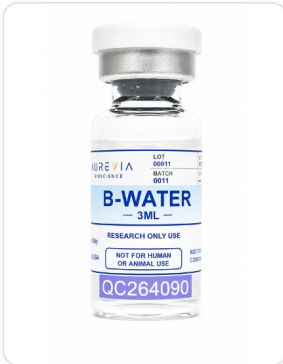

Certification: This Certificate of Analysis confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Verify authenticity at bioviridians.com/coa-search.html using the Web Verification Code above.



info@bioviridians.com

Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.